



INFRARED GAS SENSOR MIPEX-02-B-C-D.1 A (RX)

USER MANUAL

ESAT.100300.00.03 UM



INFORMATION CONTAINED IN THIS DOCUMENT IS THE SOLE PROPERTY OF SIA MIPEX. ANY REPRODUCTION IN PARTS OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF SIA MIPEX IS PROHIBITED.

Document revisions

Rev.	Date	Common changes
3.1	September 17, 2021	Change of software version to 25.8.
03	March 26, 2020	During operation, maximum surge current - 15 mA (was 10 mA) High logic level for receiving line RxD is in range of + 2.4 ... + 2.7 V (it was + 2.4 ... + 3.4). 6.4 Getting started - the value is displayed as "-0001" (was "-1") Deleted Fig. 14. Connection diagram for MIPEX-02 via MIPEX-02/03 interface board. Removed firmware 25.67 and 24.67.
02	February 21, 2020	Adding to the document CH ₄ , C ₃ H ₈ and CH ₄ /CH ₄ +C ₂ H ₆ sensors, with polycarbonate Lexan type of housings.
01	July 25th, 2018	Published version.

Table of contents

1. Introduction	4
1.1. List of abbreviations	4
1.2. List of terms	4
2. Description	5
3. Technical specifications	7
4. Intrinsic safety	9
5. Handling precautions	10
6. Installation and service	11
6.1. Preparation	11
6.2. Mounting	11
6.3. Electrical conditions	12
6.4. Getting started	15
6.5. Connecting multiple sensors to single UART line	15
7. Storage and transportation	17
8. Warranty	18
9. Contacts	19
Appendix A. Sensor types and characteristics	20
Appendix B. Connection diagram	26
Appendix C. UART communication protocol	28
Appendix C.1. General information	28
Appendix C.2. Communication protocol commands	29
Appendix C.2.1. Commands for requesting measured data	29
Appendix C.2.2. Commands for controlling operating mode	32
Appendix C.2.3. Commands for requesting factory settings and properties	32
Appendix C.2.4. Commands for sensor configuring and span calibrating	33
Appendix C.2.5. Commands for configuring net address	36
Appendix D. Sensor configuration	37
Appendix D.1. Zeroing and span calibration	37
Appendix D.2. Temperature dependence of zero adjustment	40
Appendix E. Dust filter attaching	41
Appendix F. Troubleshooting	42

1. INTRODUCTION

This user manual (UM) is intended to describe design and operation of small-sized gas sensor MIPEX-02-B-C-D.1 A (RX) (hereinafter MIPEX-02 or sensor). UM contains basic technical data, recommendations and other information necessary for proper operation, maintenance and storage of sensor.

Sensor is intended for automatic continuous measurement of carbon dioxide or hydrocarbons concentration in hazardous areas atmosphere. Sensor can be used as a part of gas-analyzing equipment of groups I and II according to IEC 60079-0, IEC 60079-11 in the explosion-hazardous zones of classes 0, 1, 2 according to IEC 60079-10-1, and Class I, Division 1, Group A, B, C, D according to UL Std. 913, CAN/CSA Std. C22.2 No.157-92. All models are suitable for equipment with temperature classes T1 – T5 at maximum ambient temperature of 60 °C.

SIA MIPEX reserves the right to make changes to this manual, excluding intrinsically safe sensor parameters.

1.1. List of abbreviations

- ADC – Analog-to-Digital Converter.
- LEL – Lower Explosive Limit.
- LED – Light Emitting Diode.
- CGM – Control Gas Mixture.
- NDIR – Non-Dispersive Infra-Red.
- UART – Universal Asynchronous Receiver/Transmitter.
- CRC – Cyclic Redundancy Check.
- IP – Ingress Protection.
- ASCII – American Standard Code for Information Interchange.
- Hex – hexadecimal.

1.2. List of terms

- Target gas is a gas, which sensor is intended to detect and measure its concentration.
- Calibration gas refers to CGM containing that gas, used for sensor calibration.

Any command stated in this UM as <X>, where X stands for a command text consisted of any number of characters, must be read and/or sent without the symbols “<” and “>”.

2. DESCRIPTION

Sensor has several modifications for specific needs. They differ by housing types, photodiode and LED, calibration gases, interface types, measuring ranges etc. (see Appendix A).

Sensor is a smart integrated system and includes mirror optical system, photodiode and LED, signal amplifiers, microcontroller, current driver of the infrared LED, UART interface signal generator and supply forming voltage unit. Sensor microcontroller performs storage of unique sensor calibration constants, processing of measurement results and concentration of measured gas, and information exchange.

Sensor operating principle is based on NDIR technology, i.e. on selective infrared radiation absorption by gas molecules.

Infrared radiation from LED permeates through a measuring diffusion-type gas cell and arrives on signal and reference photodetectors, one of which detects radiation only in the wavelength range of infrared radiation absorbed by gases, while the other one detects radiation only in the wavelength range of 3.5...3.7 μm for hydrocarbons and 4.0...4.25 μm for carbon dioxide. Gas flowing through the cell absorbs the radiation of the operating wavelength (λ_s) and does not affect the radiation of the reference wavelength (λ_{ref}). Amplitude of the photodetector operating and reference signals, U_s and U_{ref} , varies with the target gas concentration in accordance with the following equation:

$$\frac{U_s}{U_{\text{ref}}} = \exp(-[K(\lambda_s) - K(\lambda_{\text{ref}})] \cdot C \cdot L)$$

where:

$K(\lambda)$ – absorption coefficient at the predetermined wavelength;

L – optical length of the cell;

C – measured gas concentration;

U_s, U_{ref} – photodetector signals amplitude.

Differential dual wavelength method allows eliminating of water vapor, optical elements contamination and other non-selective hindrances influence.

Target gases available for MIPEX-02 are listed in Table 1.

Table 1. Target gases for MIPEX-02 sensors

Classification code (see Appendix A)	Target gas	Analytical tasks description	Spectral characteristic maximum	Notes
1	CH ₄	Analyzing a gas mixture containing methane as the main component.	3.31 μm	For optical elements sensitivity to other hydrocarbons, see Fig. 7.
2	C ₃ H ₈	Analyzing a gas mixture containing heavy hydrocarbons. The presence of methane is negligible.	3.4 μm	For optical elements sensitivity to other hydrocarbons, see Fig. 8.
3	CO ₂	Analyzing the atmosphere (including of industrial facilities) containing carbon dioxide.	4.2 μm	Sensor is selective to other gases.
4	CH ₄ /CH ₄ +C ₂ H ₆	The atmosphere of objects of group I (mine) in accordance with IEC 60079-29-1.	3.27 μm	For optical elements sensitivity to other hydrocarbons, see Fig. 9.

3. TECHNICAL SPECIFICATIONS

Table 2. General specifications (for available options see Appendix A)

Gas sampling method		Diffusion
Operating principle		Non-Dispersive Infra-Red (NDIR)
Target gas¹		CH ₄
		CH ₄ /CH ₄ +C ₂ H ₆
		C ₃ H ₈
		CO ₂
Operating, storage and transportation conditions:	Relative humidity, %	up to 98
	Atmospheric pressure, kPa	80...120
	Temperature², °C	-55...+60
Temperature range, °C		-10...+40
		-40...+60
		-20...+50
Overall dimensions, mm		∅20.3×16.6 (without pins)
Pins length, mm		4.6
Warm-up time, sec		≤ 120
Weight, g		5.5
Housing material		Plastic Lexan™
Life time expectancy³ (not less than), years		10
Shelf life time (not less than), years		8
IP rating		20 (without dust filter)
		54 (if a dust filter provided by SIA MIPEX is applied)

¹ See Appendix A for details.

² Term "operating temperature" refers to ambient temperature, at which sensor operates and its intrinsic safety is ensured, but sensor readings variability stated in


Table 3 is provided only in specified temperature range (see Table 5 and Table 6).

³ To provide metrological properties during sensor lifetime, zeroing and span calibration should be performed periodically, at least once in 30 months (see Appendix D.1).

Table 3. Measurement specifications

Measurement range, % vol.	0...1.5 (CO ₂ or C ₃ H ₈ sensors)
	0...2.5 (CH ₄ or C ₃ H ₈ sensors)
	0...5 (CH ₄ or CO ₂ sensors)
	0...100 (CH ₄ sensors)
Basic variability (+20...+25 °C)⁴	± 0.1% vol. or ± 5% of indication (whichever is greater) for CH ₄
	± 0.05% vol. or ± 5% of indication (whichever is greater) for C ₃ H ₈ and CO ₂
Response time (T90) without dust filter, sec	≤ 15
Response time (T90) when dust filter provided by SIA MIPEX is installed (see Appendix E), sec	≤ 30

Table 4. Electrical specifications, marking and standards compliance

Operating supply voltage, VDC (min...max)	+3.0...+5.0
Communication interface	UART
Average current, mA	≤ 1.1
Degree of personal protection against electrical shock caused by sensor	meets the requirement of class III ГОСТ 12.2.007.0
Marking and standards compliance	Ex ia I Ma U/Ex ia IIC Ga U acc. to ГОСТ 31610.0-2014, ГОСТ 31610.11-2012, TP TC 012/2011
	Ex ia I Ma/Ex ia IIC Ga acc. to IEC 60079-0, IEC 60079-11. -55 ≤ Ta ≤ +60 °C
	IM 1/II 1 G Ex ia I Ma/Ex ia IIC Ga acc. to EN 60079-0, EN 60079-11. -55 ≤ Ta ≤ +60 °C
	<p>RECOGNIZED COMPONENT</p>  <p>Class I, Division 1, Group A, B, C, D CONFORMS TO UL Std. 913, 60079-0, 60079-11 CERT. TO CAN/CSA Std. C22.2 No. 157-92</p>

⁴ For variability in the whole operating temperature range for any sensor modification, see Table 6.

4. INTRINSIC SAFETY

Sensor's intrinsic safety is provided by:

- limiting parameters of its electrical circuits to intrinsically safe values in accordance with IEC/EN 60079-11;
- providing the required electrical clearances and creepage paths in accordance with IEC/EN 60079-11;
- insulation between intrinsically safe circuit and sensor housing, which withstands test voltage of 500 V in accordance with EN 60079-11.

Combined intrinsically safe sensor circuits parameters:

- IECEx/ATEX: $U_i = 5.0 \text{ V}$, $I_i = 450 \text{ mA}$, $P_i = 0.25 \text{ W}$, $C_i = 38.8 \text{ }\mu\text{F}$, $L_i = 0 \text{ mH}$.
- CAN/CSA: $V_{\text{max}} = 5.0 \text{ V}$, $I_{\text{max}} = 450 \text{ mA}$, $P_{\text{max}} = 0.25 \text{ W}$, $C_i = 38.8 \text{ }\mu\text{F}$, $L_i = 0 \text{ mH}$.

It is allowed to connect sensor only to intrinsically safe circuits with the rated direct current output voltage (U_0) within the range of +3.0...+5.0 V, with the output power (P_0) range of 0.02...0.25 W in accordance with IEC 60079-0, IEC 60079-11, IEC 60079-14 and whose parameters conform MIPEX-02 intrinsic safety values pointed above. Current provided by power supply unit must be $25 \text{ mA} \leq I_0 \leq 450 \text{ mA}$.

5. HANDLING PRECAUTIONS

- Do not use damaged sensor. It must be repaired only by personnel authorized by manufacturer.
- Keep sensor out of contact with aggressive substances e.g. acidic environments, which can react with metals, as well as solvents, which may affect polymeric materials.
- Diffusion holes of sensor should be protected against ingress of dust and sprayed materials.
- Sensor is not intended to measure target gas concentration contained in fluids.
- Maximum allowable pressure on the central part of sensor reflecting cover or to sensor side surface – 20 kPa, on sensor upper edge – 2 MPa.
- Sensor updates information about concentration every 1.28 ± 0.065 seconds. Sending any command more often than one time per second (1 Hz) may reduce sensor accuracy.
- Sensor may accumulate an electrostatic charge on its housing. Thus, there is risk of electrostatic discharge. Clean only using a damp cloth.
- Correct measurement is provided when ambient temperature changes not faster than 0.6 °C/min.
- Covering diffusion holes of sensor increases its response time (T90).
- When operating sensor, observe conditions stated in Table 2 and Table 4.
- Inspection and maintenance should be carried out by suitably trained personnel in accordance with the applicable code of practice (e.g. EN 60079-17).
- Persons, who have studied this UM, must be briefed on safety precautions when operating electrical equipment intended for use in explosive areas in due course.
- When dealing with cylinder containing gas mixture under pressure, it is necessary to follow the safety regulations. Dumping of CGM into the work area is not allowed.
- There is no risk of pollution and negative impact on human health. Sensor does not contain any harmful substances that may be released during its normal operation.
- It is strictly prohibited to remove label from sensor or to damage marking information in any way.

6. INSTALLATION AND SERVICE



- Sensor may accumulate an electrostatic charge on its housing. Thus, there is risk of electrostatic discharge. Clean only using a damp cloth. Note this during installation and use of sensor in the end-user equipment.
- Sensor must be mounted using sockets only, as soldering the pins may damage sensor.
- It is not allowed to use excessive pressure on sensor housing. Maximum allowable pressure on the central part of sensor reflecting cover or on sensor side surface – 20 kPa, on sensor upper edge – 2 MPa.
- Span calibration is necessary during sensor's initial installation into gas analyzers and during preparation for the equipment checking. Manual zeroing must be performed after prolonged storage without power supply, after transportation as well as after dust filter is applied (see Appendix D.1).
- It is required to perform span calibration at least once in 30 months.

6.1. Preparation

- If sensor has been kept in transport containers at temperatures below zero centigrade, leave it at +10...+35 °C for not less than one hour.
- Remove the packaging. Check presence of the certification markings; make sure there are no mechanical injuries on sensor surfaces.

6.2. Mounting

Use intrinsically safe circuit connections represented in Appendix B.

It is recommended to use the following sockets or similar for sensor mounting:

- Cambion 450-3729-01-06-00;
- Harwin H3183-05;
- Harwin H3182-05

Sensor pinout is shown in Appendix A,

Table 7.

End user instrument design has to provide that sensor is free of excessive pressure on its housing, ingress of dust, dirt and condensed moisture, as these factors may affect the accuracy of measurement. It is recommended to use dust filter (available as an option; see Appendix E). Filter has to be checked regularly and replaced when fouling is significant.

6.3. Electrical conditions



- During first 0.01 seconds after power up, sensor consumes up to 55 mA, and then during 0.1 second average current consumption up to 14 mA (see Fig. 1). After that sensor switches to the normal current consumption mode.
- During operation, MIPEX-02 has pulsed current consumption. Pulse repetition period is $80 \pm 20\%$ ms (depends on ambient temperature).
- During operation, maximum surge current is 17 mA for 20 microseconds (see Fig. 2). Average current consumption is not more than 330 μ A when UART is active (see Fig. 3). For power consumption of sensor connected via barrier see Fig. 4 and Fig. 5.

Use intrinsically safe circuit connections represented in Appendix B.

Sensor power supply has to follow requirements of IEC 60079-0 and IEC 60079-11, with rated output range of intrinsically safe DC voltage (U_0) of +3.0...+5.0 V, with rated power range (P_0) of 0.02...0.25 W. Current provided by power supply unit must be $25 \text{ mA} < I_0 \leq 450 \text{ mA}$.

End-user equipment UART transceiver should meet the requirements of standards IEC 60079-0, IEC 60079-11.

Sensor UART transceiver communication properties are:

- High logic level for transmitting line TxD is in range of +2.4...+2.7 V;
- High logic level for receiving line RxD is in range of +2.4...+2.7 V;
- Low logic level is in range of 0...+0.8 V;
- Maximum output current of UART is not more than 25 mA.

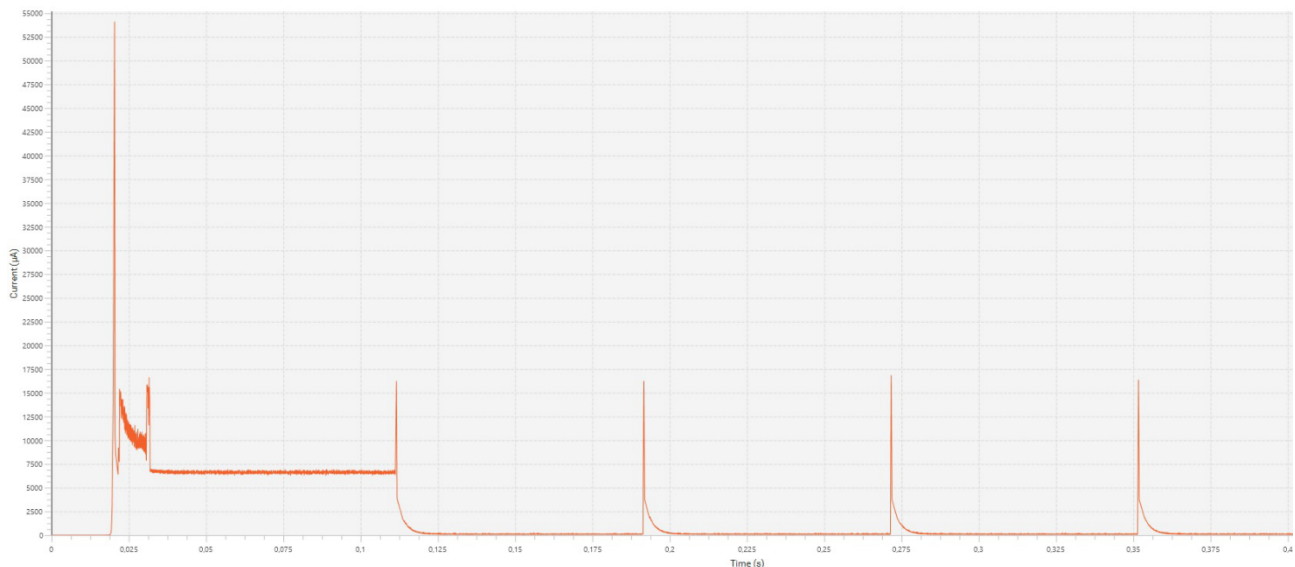


Fig. 1. Typical current consumption waveform after power up

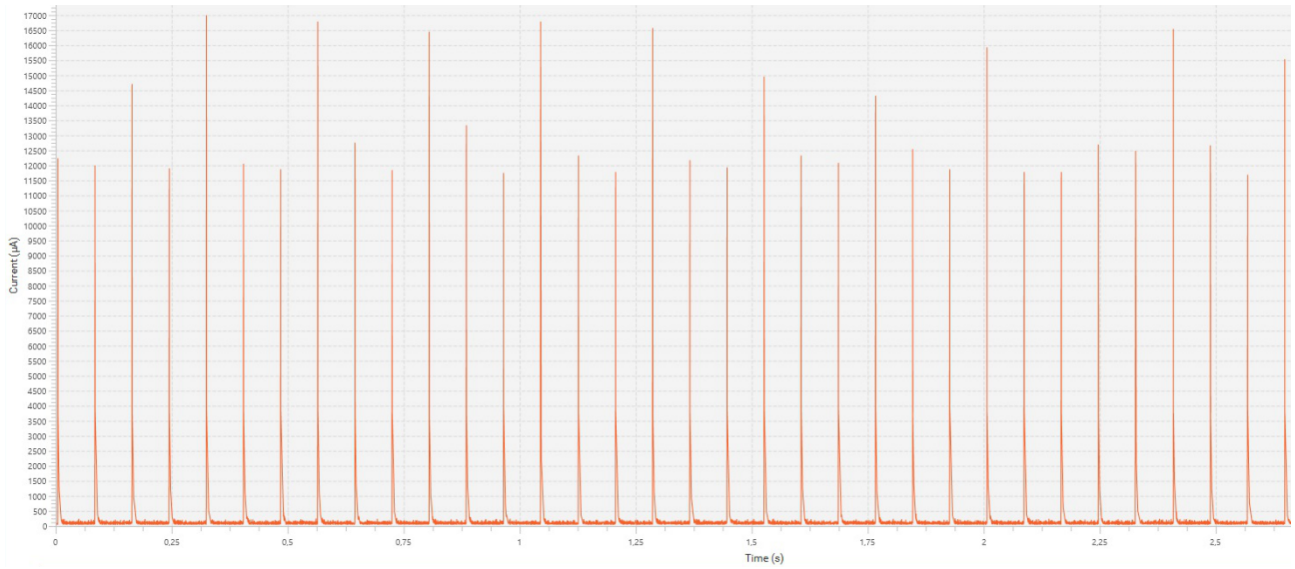


Fig. 2. Typical current consumption waveform

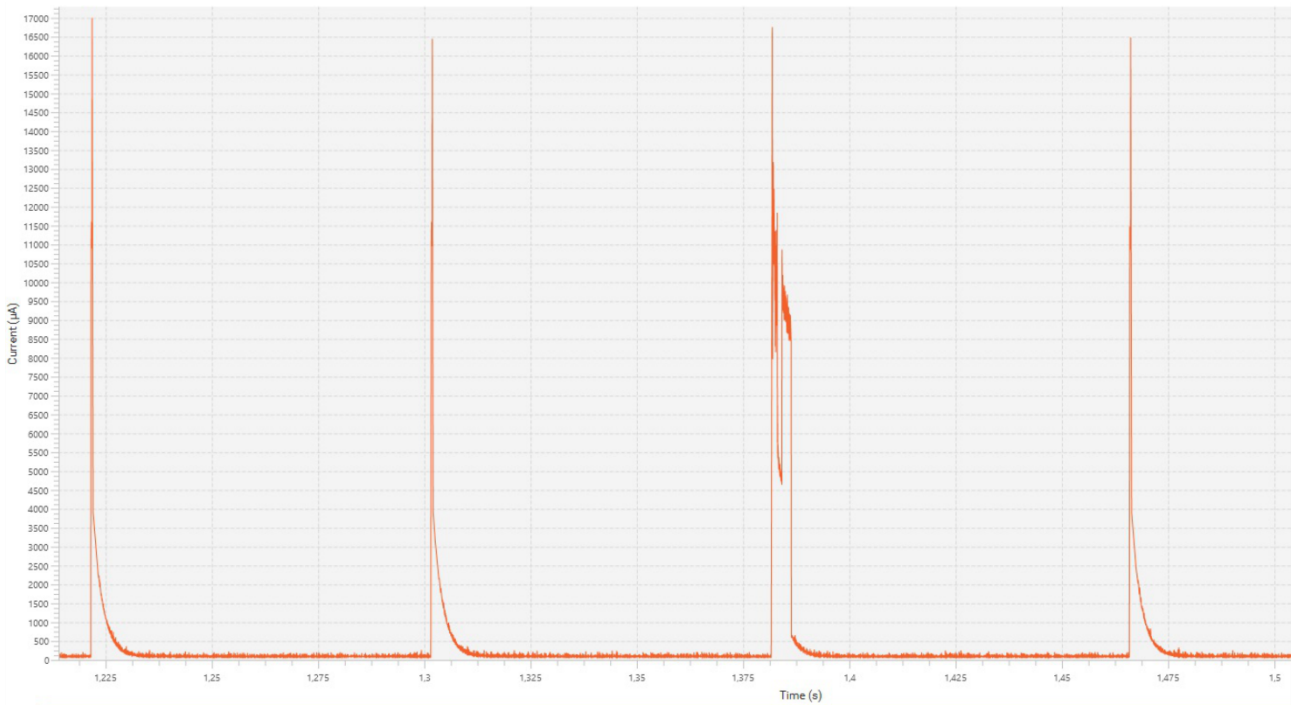


Fig. 3. Typical current consumption waveform when UART is active (<@> command)

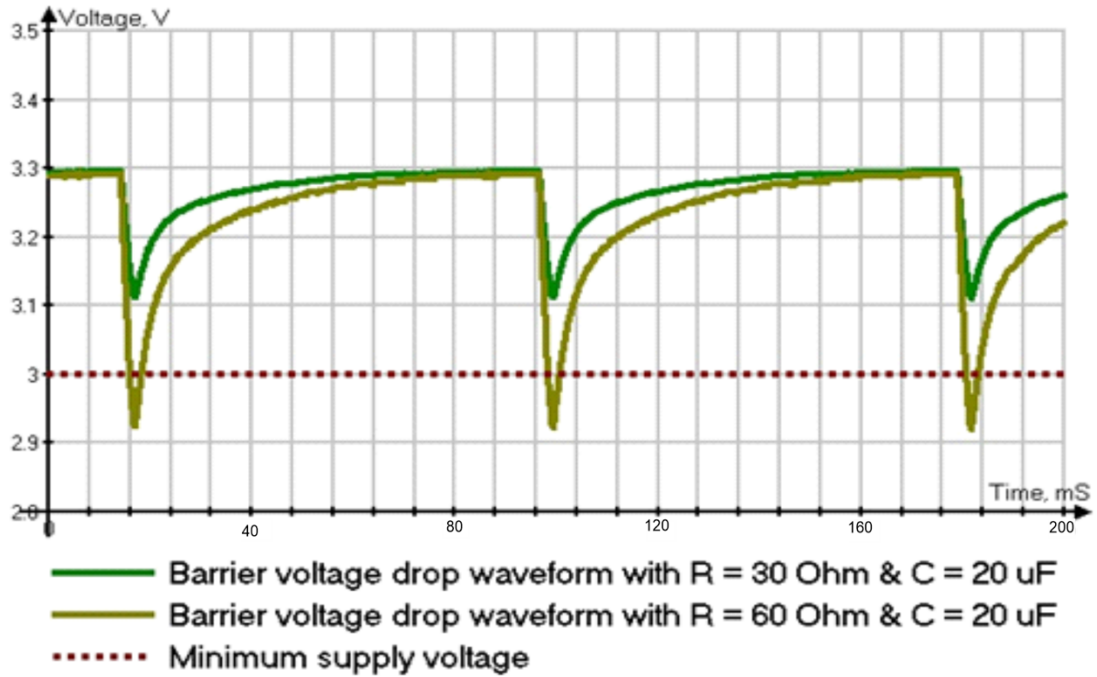


Fig. 4. Typical barrier voltage drop waveform (3.3 V input)

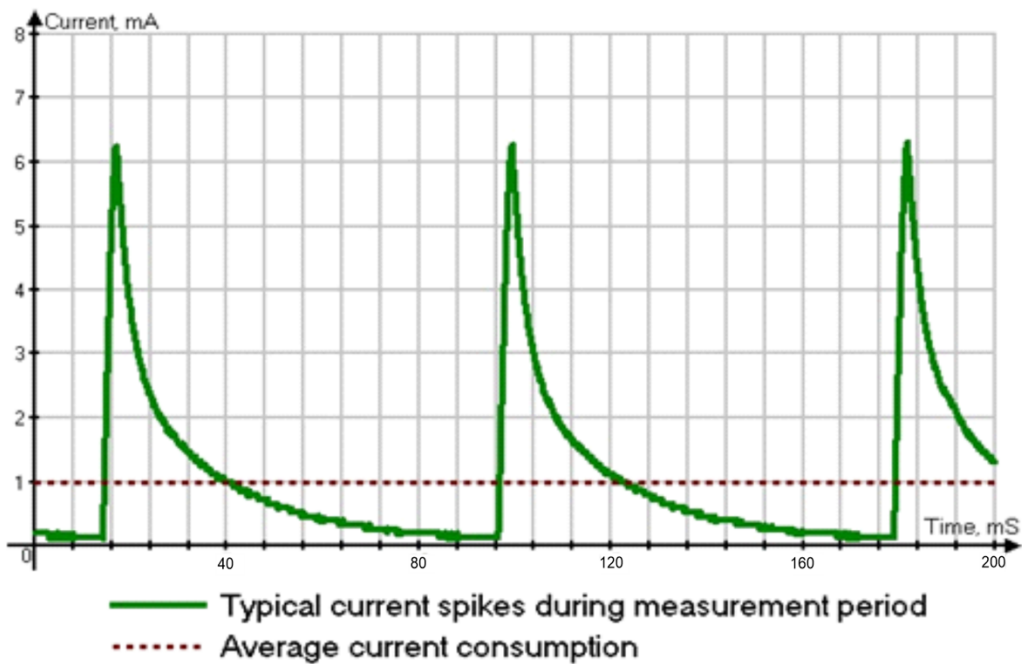


Fig. 5. Typical current consumption waveform (3.3 V input, R = 30 Ohm, C = 20 uF)

6.4. Getting started



- During first 40 seconds after the power is up sensor does not return the measured concentration value (the value is displayed as “-0001”, hex: “8001”, see Table 13).
- When the measurement range is exceeded, concentration value is displayed as “32767” (hex: “7FFF”).
- Sensor updates information about concentration every 1.28 ± 0.065 seconds. Sending any command more often than one time per second (1 Hz) may reduce sensor accuracy.

Switching on/off sensor is performed automatically upon feeding/disconnecting power supply.

After sensor is installed into end-user equipment check its status by sending <DATAE2> command via UART interface:

- for <DATAE2> command description see Appendix C.2.1;
- for status bytes description and recommendations see Table 12.

Sensor span calibration and zeroing should be performed next. Methods of sensor span calibration and zeroing are given in Appendix D.1.

6.5. Connecting multiple sensors to single UART line

It is possible to connect to single UART line up to 256 sensors assigning them net addresses in range 00...FF. Sensor has net address 00 by default. To view and change its net address use the following commands: <!*>, <NETON>, <NETOFF>, <%AABB>. For commands description see Appendix C.2.5.

If sensor is used in combination with other devices on single UART line, any command text must contain sensor's address prefix as “#AA”, where AA stands for sensor's net address in hexadecimal format in range 00...FF. Thus, command text must be sent as <#AAX>, where X stands for command text containing any number of characters in accordance with sensor communication protocol (see Appendix C). Connection diagram of multiple sensors to single UART line is shown on Fig. 6.

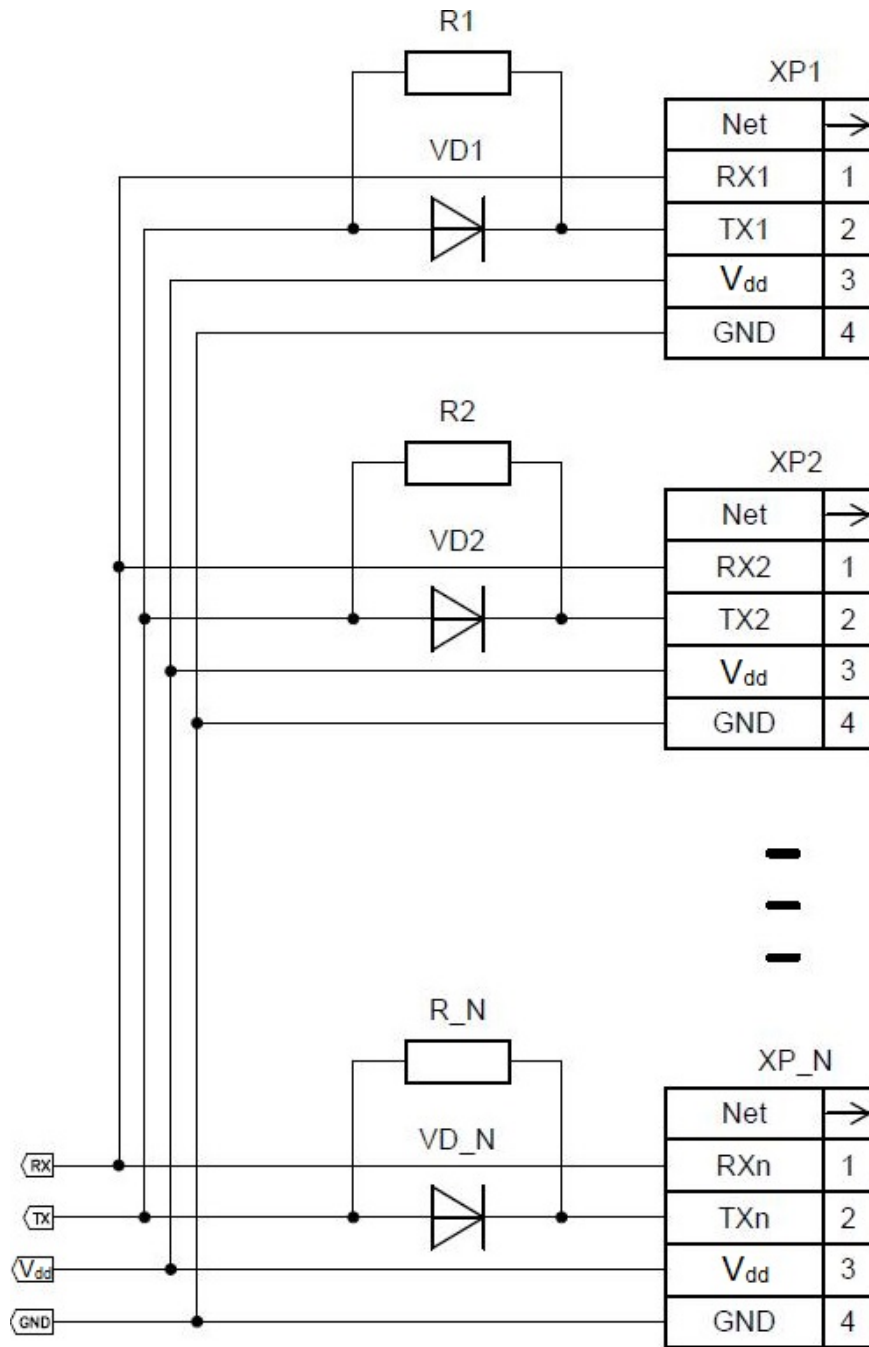


Fig. 6. Connection diagram of multiple sensors to single UART line

Resistors are calculated as follows:

1. Determine the quantity of sensors N that should be connected to single UART line.
2. Determine forward voltage U_f of Schottky diodes (VD_N).
3. Calculate the minimum allowed resistance R_{min} by using the following equation:

$$R_{min} = \frac{U_h - U_f}{I_{out}} \times (N - 1),$$

where:

U_h – maximum high logic level voltage (2.7 V);

I_{out} – maximum output current of sensor microcontroller (25 mA).

7. STORAGE AND TRANSPORTATION

Transportation can be done by all means of transportation in covered vehicles as well as in a heated pressurized plane compartments in accordance with the rules of cargoes transportation actual for the respective type of transportation.

Sensor in manufacturer's package should be kept in supplier and customer's storages under storage conditions specified in Table 2. Ambient atmosphere should be free of any harmful impurities that can cause corrosion.

8. WARRANTY

Manufacturer guarantees sensor compliance with specifications and requirements stated in this UM if customer follows operating, transportation and storage terms.

During warranty period, manufacturer replaces or repairs for free all its products that do not operate because of production fault.

Warranty period is 24 months since product is shipped to customer. Shipment date is registered in the ESAT.100300.00 PS manufacturer's certificate.

Manufacturer is not responsible for sensor fault and discontinues warranty in following cases:

- if the rules and conditions of operation, transportation and storage stated in this UM and in sensor datasheet were violated;
- if sensor has marks of unauthorized repair attempts;
- if any mechanical damage occurs and/or if any damage is caused by exposure to extremely high or low temperatures, corrosion, oxidation, ingress of any foreign objects, materials, liquids, insects;
- if sensor was damaged by using connection circuit that does not comply with requirements stated in this UM;
- if damage is caused by force majeure, accident, intentional or careless actions of the customer or third parties;
- if damage (or fault) is caused by installing, editing or damaging sensor firmware and/or by making changes to the firmware settings using service codes;
- if damage (or fault) is caused by the fact of power and signal cables do not meet the standard or technical regulations and/or by electromagnetic interferences exceeding permissible according to EN 60079-29-1.

Replacement or repairs of faulty sensor does not extend initial warranty period.

Manufacturer is not responsible for any possible damage directly or indirectly caused by sensor to people and property in case it is a result of improper usage, storage and transportation or due to intentional or careless actions of the customer and/or third parties.

Risks and costs of transportation and packaging as well as other contingencies concerning product return to manufacturer are carried out by the customer.

For warranty information or additional assistance, please contact support service (see Chapter 9).

9. CONTACTS

MIPEX TECHNOLOGY

SIA MIPEX

2B, Valkas iela, Daugavpils, Latvia, 5417

Tel/fax: +371 26179021


web: www.mipex-tech.com

e-mail: info@mipex-tech.com

support: support@mipex-tech.com

APPENDIX A. SENSOR TYPES AND CHARACTERISTICS

MIPEX-02-B-C-D.1 X (RX)

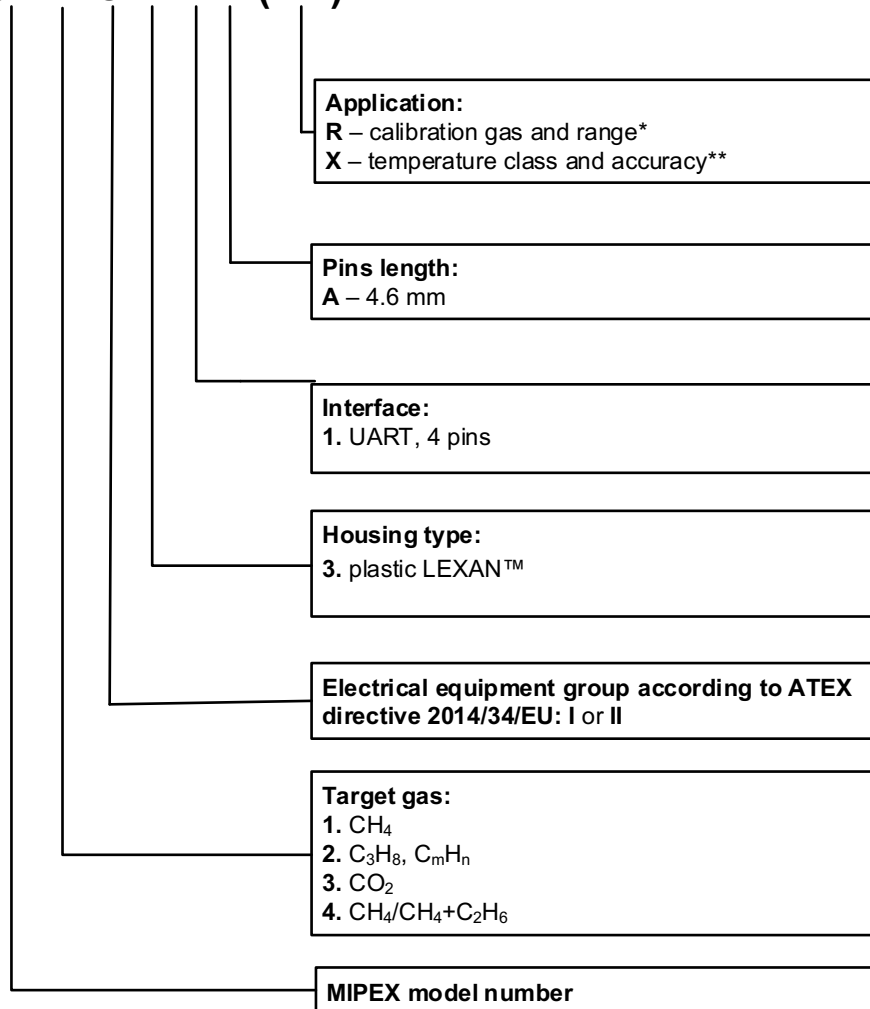

* See Table 5 for details.

** See Table 6 for details.

Table 5. Metrological properties of sensor (RX-code)

Part number	Target gas ⁵	Calibration gas	Meas. range, % vol.	Temp. range, °C	RX	
MIPEX-02-1-I-D.1 X (00)	CH ₄	CH ₄	0...2.5	-10...+40	00	
MIPEX-02-1-I-D.1 X (10)			0...5		10	
MIPEX-02-1-I-D.1 X (20)			0...100		20	
MIPEX-02-1-II-D.1 X (01)			0...2.5	-40...+60	01	
MIPEX-02-1-II-D.1 X (11)			0...5		11	
MIPEX-02-1-II-D.1 X (21)			0...100		21	
MIPEX-02-1-II-D.1 X (02)		0...2.5	-20...+50	02		
MIPEX-02-1-II-D.1 X (12)		0...5		12		
MIPEX-02-1-II-D.1 X (22)		0...100		22		
MIPEX-02-1-II-D.1 X (61)		C ₃ H ₈	C ₃ H ₈	0...1.5	-40...+60	61
MIPEX-02-1-II-D.1 X (71)				0...2.5		71
MIPEX-02-1-II-D.1 X (62)				0...1.5	-20...+50	62
MIPEX-02-1-II-D.1 X (72)				0...2.5		72
MIPEX-02-2-II-D.1 X (61)		C ₃ H ₈	C ₃ H ₈	0...1.5	-40...+60	61
MIPEX-02-2-II-D.1 X (71)	0...2.5			71		
MIPEX-02-2-II-D.1 X (62)	0...1.5			-20...+50	62	
MIPEX-02-2-II-D.1 X (72)	0...2.5				72	
MIPEX-02-3-I-D.1 A (30)	CO ₂	CO ₂	0...1.5	-10...+40	30	
MIPEX-02-3-II-D.1 A (32)				-20...+50	32	
MIPEX-02-3-I-D.1 A (40)			0...5	-10...+40	40	
MIPEX-02-3-II-D.1 A (42)				-20...+50	42	
MIPEX-02-4-I-D.1 X (00)	CH ₄ / CH ₄ +C ₂ H ₆	CH ₄	0...2.5	-10...+40	00	
MIPEX-02-4-I-D.1 X (10)			0...5		10	
MIPEX-02-4-I-D.1 X (20)			0...100		20	
MIPEX-02-4-II-D.1 X (01)			0...2.5	-40...+60	01	
MIPEX-02-4-II-D.1 X (11)			0...5		11	
MIPEX-02-4-II-D.1 X (21)			0...100		21	
MIPEX-02-4-II-D.1 X (02)			0...2.5	-20...+50	02	
MIPEX-02-4-II-D.1 X (12)			0...5		12	
MIPEX-02-4-II-D.1 X (22)			0...100		22	

⁵ Typical sensor sensitivity to other hydrocarbons is shown on Fig. 7, Fig. 8 and Fig. 9.

Table 6. Basic sensor readings variability⁶

Calibration gas	Readings variability within a temperature range	Additional variability due to pressure	Additional variability due to humidity
CH ₄	±0.1% vol. or ±5% of indication (whichever is greater) within the range of +20...+25 °C;	±0.2% vol. or ±30% of indication (whichever is greater) at 100 kPa (test: 80 kPa, 100 kPa, 120 kPa)	±0.2% vol. or ±15% of indication (whichever is greater) at 40 °C (test: 20% RH, 50% RH, 90% RH)
	±0.2% vol. or ±10% of indication (whichever is greater) within the range of -10...+20 °C and +25...+40 °C;		
	±0.4% vol. or ±20% of indication (whichever is greater) within the range of -40...-10 °C and +40...+60 °C.		
C ₃ H ₈	±0.05% vol. or ±5% of indication (whichever is greater) within the range of +20...+25 °C;	±0.1% vol. or ±30% of indication (whichever is greater) at 100 kPa (test: 80 kPa, 100 kPa, 120 kPa)	±0.1% vol. or ±15% of indication (whichever is greater) at 40 °C (test: 20% RH, 50% RH, 90% RH)
	±0.1% vol. or ±10% of indication (whichever is greater) within the range of -10...+20 °C and +25...+40 °C;		
	±0.2% vol. or ±20% of indication (whichever is greater) within the range of -40...-10 °C and +40...+60 °C.		
CO ₂	± 0.05% vol. or ± 5% of readings (whichever is greater) within the range of +20...+25 °C;	± 0.1% vol. or ± 40% of readings (whichever is greater) at 100 kPa (tested at 80 kPa, 100 kPa, 120 kPa)	± 0.1% vol. or ± 15% of readings (whichever is greater) at 40 °C (tested at 20% RH, 50% RH, 90% RH)
	± 0.1% vol. or ± 10% of readings (whichever is greater) within the range of -10...+20 °C and +25...+40 °C;		
	± 0.2% vol. or ± 20% of readings (whichever is greater) within the range of -20...-10 °C and +40...+50 °C.		

⁶ The table shows basic variability of MIPEX-02 sensor readings. For each sensor modification, readings variability stated in Table 6 is provided within a temperature range determined by a sensor RX-code (see Table 5).

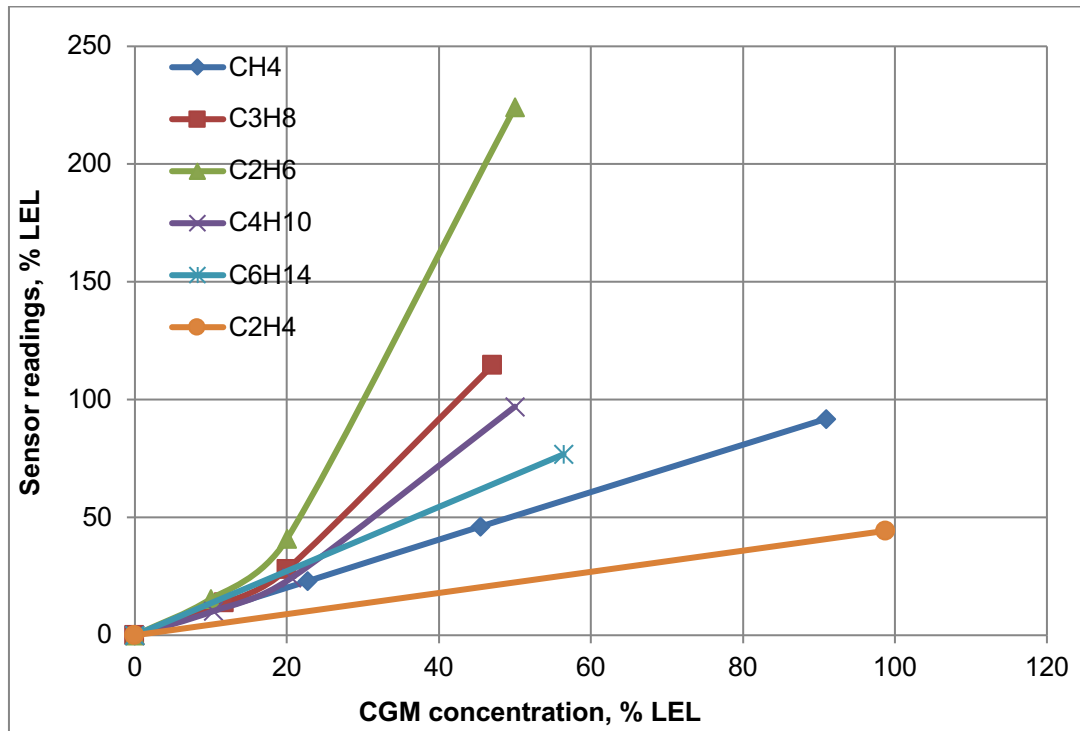


Fig. 7. Typical sensitivity of MIPEX-02-1-X-X.1 X (target and calibration gas is CH₄) to other hydrocarbons

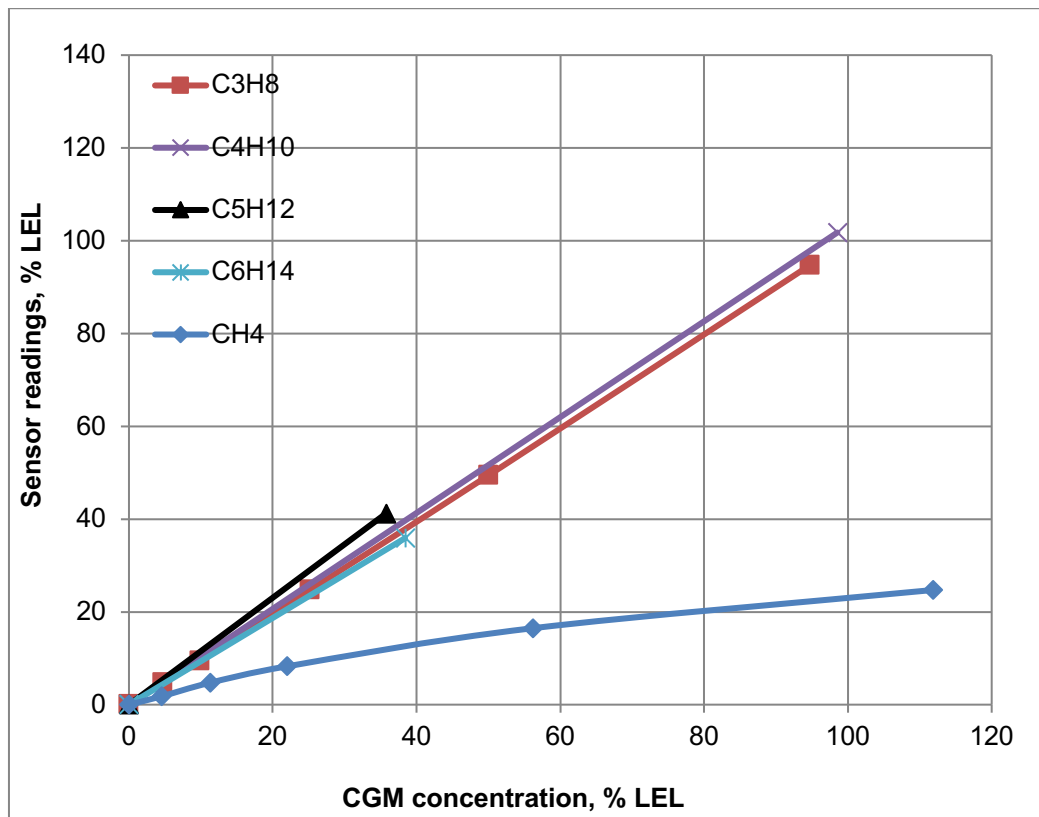


Fig. 8. Typical sensitivity of MIPEX-02-2-X-X.1 X (target and calibration gas is C₃H₈) to other hydrocarbons

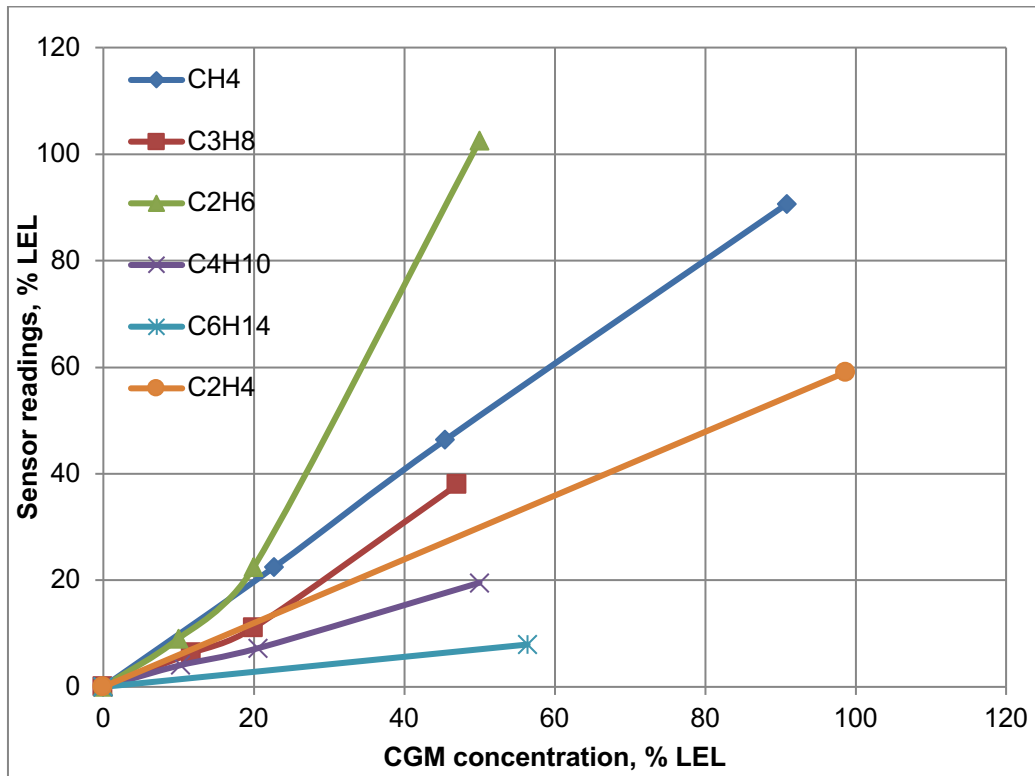


Fig. 9. Typical sensitivity of MIPEX-02-4-X-X.1 X (target gas is CH₄/CH₄+C₂H₆ and calibration gas is CH₄) to other hydrocarbons


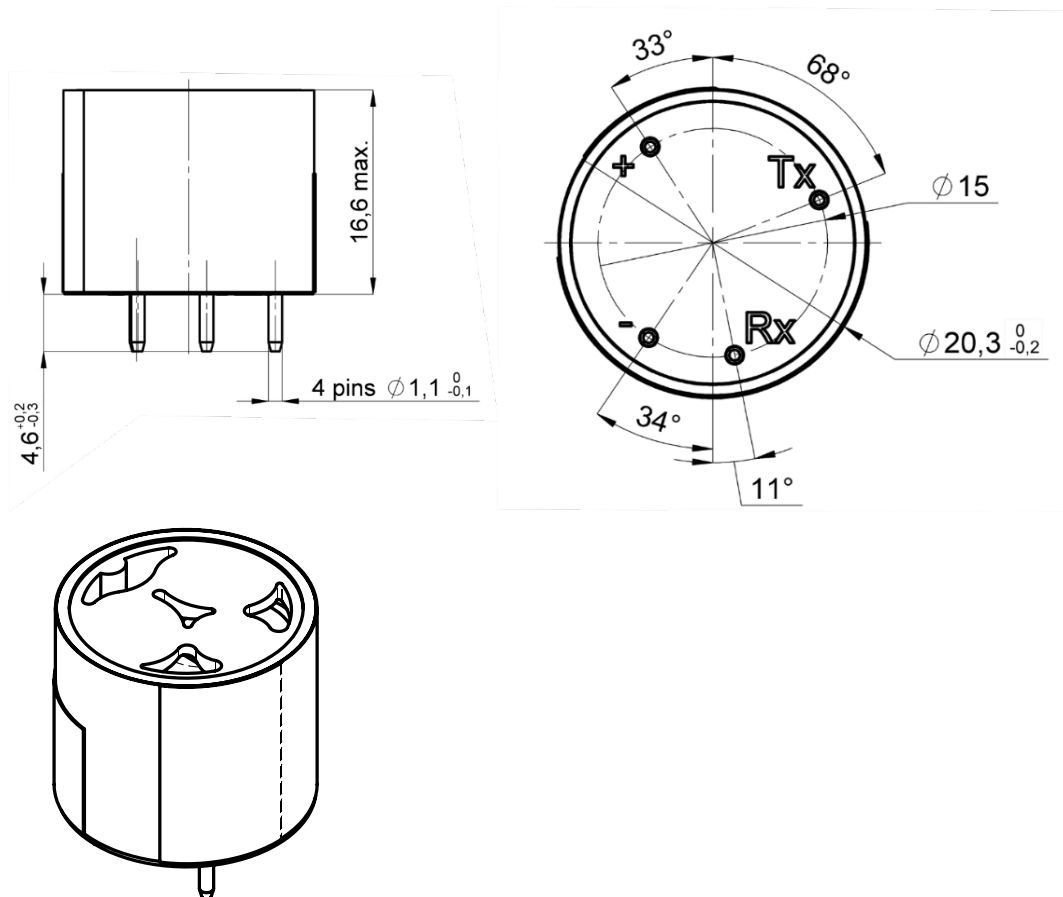


Fig. 10. MIPEX-02-B-C-3.1 A (housing type “3”) overall dimensions in millimeters

Table 7. Sensor pinout

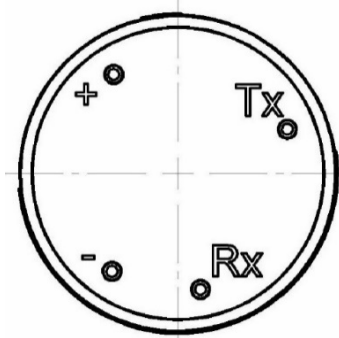

Pin	Purpose
Tx	UART, TxD output
Rx	UART, RxD input
+	V _{dd}
-	GND

APPENDIX B. CONNECTION DIAGRAM

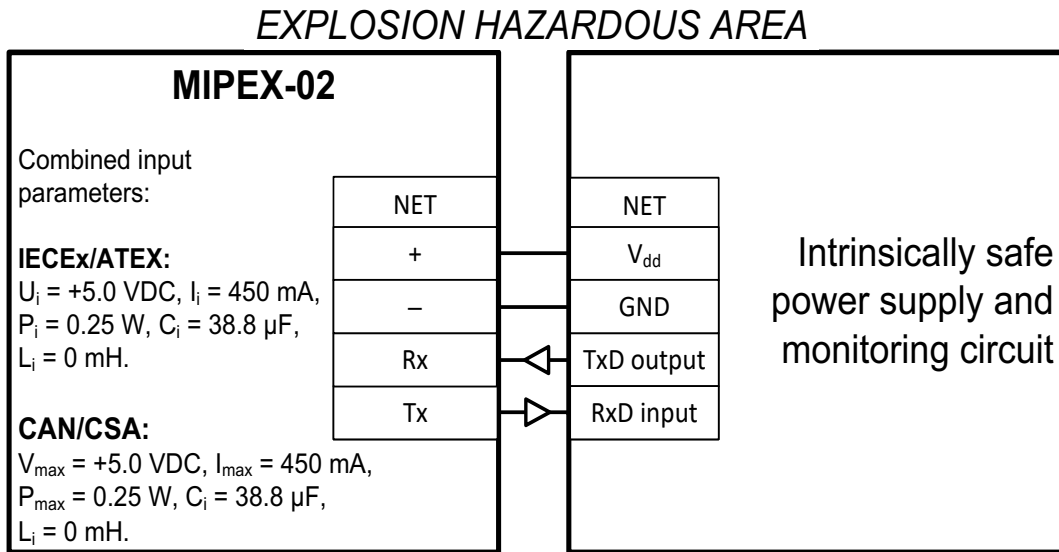


Fig. 11. Connection diagram for MIPEX-02

EXPLOSION HAZARDOUS AREA

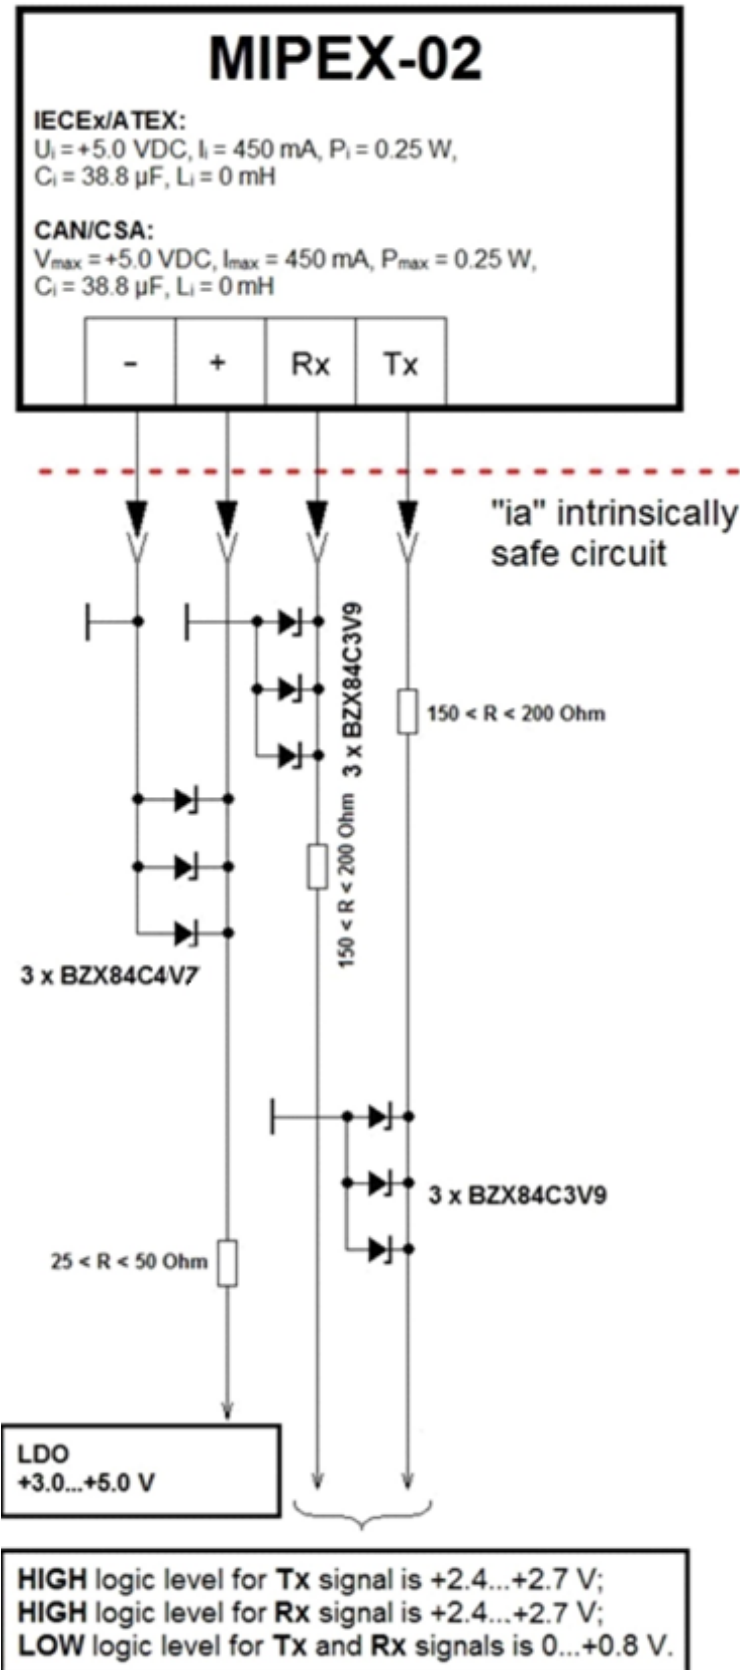


Fig. 12. Example of connecting MIPEX-02 to "ia" intrinsically safe circuit

APPENDIX C. UART COMMUNICATION PROTOCOL

Current manual describes firmware releases 25.8. Sensor communication protocol is based on UART interface. Contact support service for available compatible versions and instructions.

Appendix C.1. General information

Data exchange with MIPEX-02 sensors is performed via UART interface:

- Sensor has symbol rate of 9600 baud.
- Data format: 8-bit message, 1 stop bit, no parity checking.
- Electrical parameters of UART are pointed in section 6.3.

General command format:

- any command stated in this UM as <X>, where X stands for a command text consisted of any number of characters, must be read and/or sent without the symbols "<" and ">";
- ASCII code for commands and most responses;
- command ends with carriage return symbol (hex: "0D");
- words and/or values in a response on most commands are separated by space symbol (hex: "20") or in some cases by tabulation (hex: "09");
- all symbols in command must be sent as one word without delays;
- sensor does not respond to incorrectly sent commands;
- sensor has two operating modes (access levels): "OEM" and "USER"; "OEM" has extended command set for developers, while "USER" mode is used for field operations;
- if sensor is used in combination with other devices on single UART line, then to refer to a specific sensor, before any command from the communication protocol must write prefix as "#XX", where XX stands for sensor's net address in hexadecimal format in range 00...FF. The assignment of the net address to the sensor is described in chapter 6.5. Example of writing the command #XXINDSIG ON and responding to this command #XXINDSIG ON OK.



When accessing the sensor using commands from the communication protocol for writing / rewriting data into the sensor's memory, do not turn off the sensor power supply within 2 seconds after the submission of the corresponding commands from the communication protocol.

Appendix C.2. Communication protocol commands

There are several types of commands used for communication with sensor:

1. commands for requesting measured data and diagnosing (see Appendix C.2.1);
2. commands for controlling operating mode (see Appendix C.2.2);
3. commands for requesting factory settings and properties (see Appendix C.2.3);
4. commands for sensor configuring and span calibration (see Appendix C.2.4);
5. commands for configuring net address (see Appendix C.2.5);



- Always check command syntax before sending. Commands that are not listed in this user manual are prohibited. Otherwise, it may result in malfunction of sensor.
- In earlier versions of the firmware, some commands are unavailable.

Appendix C.2.1. Commands for requesting measured data

There are five commands available for user to request concentration value. Primary command to request measured data is <@*X> as it requires minimum power to process it.

Request syntax	USER mode	OEM mode	Response description	Command description
@	yes	yes	2 bytes in binary format (see Table 8).	Returns sensor readings of scaled concentration C_1 (not periodically, single time only).
@*X	yes	yes	"@" symbol in ASCII format and 2 bytes in binary format (see Table 8).	Returns sensor readings of scaled concentration C_1 periodically (every $[1.28 \pm 0.065] \times X$ sec), where X is a value within the range 0...9 in ASCII format).
CCS	yes	yes	5 bytes in ASCII format and "0D" symbol.	Returns sensor current ambient temperature in Celsius degrees.
CFS	yes	yes	5 bytes in ASCII format and "0D" symbol.	Returns sensor current ambient temperature in Fahrenheit degrees.
CKS	yes	yes	5 bytes in ASCII format and "0D" symbol.	Returns sensor current ambient temperature in Kelvins.
DATA	yes	yes	5 bytes in ASCII format and "0D" symbol (see Table 9).	Returns sensor readings of scaled concentration C_1 .
DATAE	yes	yes	4 bytes in binary format and "0D" symbol (see Table 10).	Returns sensors readings of scaled concentration C_1 , status byte and CRC value.
DATAE2	yes	yes	5 bytes in binary format and "0D" symbol (see Table 11).	Returns sensor readings of scaled concentration C_1 , two status bytes and CRC value.

Table 8. Structure of response on <@> and <@*X> commands

	Command <@> (hex: "40 0D")		Command <@*X> (hex: "40 2A X 0D")		
Byte number	1	2	1	2	3
Byte data ⁷	C ₁ H	C ₁ L	@ (hex: "40")	C ₁ H	C ₁ L

Table 9. Structure of response to <DATA> command

	Command <DATA> (hex: "44 41 54 41 0D")	
Byte number	1-5	6
Byte data	C ₁	hex: "0D"

Table 10. Structure of response to <DATAE> command

	Command <DATAE> (hex: "44 41 54 41 45 0D")				
Byte number	1	2	3	4	5
Byte data ⁸	C ₁ H	C ₁ L	StatusByte	CRC	hex: "0D"

Table 11. Structure of response to <DATAE2> command

	Command <DATAE2> (hex: "44 41 54 41 45 32 0D")					
Byte number	1	2	3	4	5	6
Byte data ⁹	C ₁ H	C ₁ L	StatusByteH	StatusByteL	CRC	hex: "0D"

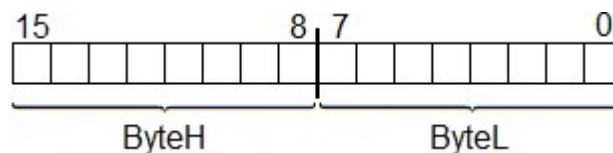


Fig. 13. High and low bytes structure

⁷ High and low bytes structure is presented on Fig. 13.

⁸ If bits of status byte are true, check their meanings in Table 12 and perform recommended operations.

⁹ If bits of status bytes are true, check their meanings in Table 12 and perform recommended operations.

High and low bytes structure is presented on Fig. 13.

Table 12. Bits of status bytes description

Bit number of <DATAE2> status-bytes	Bit number of <DATAE> status-byte	Description	Recommendations
–	–	Normal mode, static temperature	–
0	0	Sensor is warming up.	Do not perform span calibration.
1	1	An abrupt signal change (due to feeding a gas mixture to sensor atmosphere) or increased noise on sensor optical elements.	Do not perform span calibration or zeroing. If this status longer than for 20 minutes at stable conditions, replace sensor.
2	2	One of the signal values is lower than it is allowed.	Possibility of condensed moisture on optical elements. Dry sensor. After drying, if this status lasts longer than for 20 minutes at stable conditions, replace sensor.
3	3	reserved	Does not contain any significant information.
4	4	Dynamic temperature mode (temperature changes faster than by 0.6 °C/min).	Do not perform span calibration or zeroing.
5	5	Dynamic temperature mode (temperature changes faster than by 2 °C/min).	Do not perform span calibration or zeroing.
6	6	Exceeding temperature limits.	Check the ambient temperature.
7	7	Firmware failure (flash memory issues).	Contact support for details.
8	–	Data request rate is more than 1 Hz.	Do not perform span calibration or zeroing. Decrease request rate.
9	–	Zero shifts to negative value.	Possibility of condensed moisture on optical elements. Dry sensor. After drying, if this status lasts longer than for 20 minutes at stable conditions, perform zeroing (see Appendix D.1 for procedure description).
10	–	Sensor operates in low power consumption mode.	–
11	–	Complex status. Technological failure.	Contact support for details.
12	–	reserved	Does not contain any significant information.
13	–	reserved	Does not contain any significant information.
14	–	reserved	Does not contain any significant information.
15	–	reserved	Does not contain any significant information.
(4 v 5) & 9	–	Dynamic temperature mode; zero shifts to negative value.	Do not perform span calibration or zeroing.

Appendix C.2.2. Commands for controlling operating mode

Request syntax	USER mode	OEM mode	Response description	Command description
OEM XXXX	yes	no	Response contains of word "OEM" or, if the password is incorrect, word "USER" in ASCII format and "0D" symbol.	Switches commands level from "USER" to "OEM"; XXXX stands for current password. Default password is 0000.
PASS?	no	yes	Response contains of 4 bytes in ASCII format and "0D" symbol.	Returns current password for switching commands level from "USER" to "OEM".
PASS XXXX YYYY	no	yes	PASS XXXX YYYY OK or PASS XXXX YYYY FAULT	Intended for changing current password for switching commands level from "USER" to "OEM". XXXX stands for old password and YYYY stands for new one. New password should contain only digits 0...9 in ASCII format.
UART?	yes	yes	USER or OEM	Returns active access level.
USER	no	yes	Response contains of word "USER" in ASCII format and "0D" symbol.	Switches commands level from "OEM" to "USER".

Appendix C.2.3. Commands for requesting factory settings and properties

Request syntax	USER mode	OEM mode	Response description	Command description
ID?	yes	yes	Summary info in ASCII format about sensor type, its serial number, characteristics and firmware version.	Returns sensor ID.
RT?	yes	yes	5 bytes in ASCII format and "0D" symbol (the codes list is available upon query).	Returns sensor type.
RX?	yes	yes	2 bytes in ASCII format and "0D" symbol. See Table 5 for details.	Returns sensor characteristics (temperature class, calibration range and accuracy).
SRAL?	yes	yes	8 bytes in ASCII format and "0D" symbol.	Returns sensor serial number (SN).
SREV?	yes	yes	Sensor firmware version.	Returns the firmware version.

Appendix C.2.4. Commands for sensor configuring and span calibrating

Request syntax	USER mode	OEM mode	Response description	Command description
AZERO?	no	yes	AZERO ON or AZERO OFF	Intended for checking current auto-zeroing algorithm status (this algorithm must not be used on CO ₂ sensors).
AZERO OFF	no	yes	AZERO OFF OK	Turns off the auto-zeroing algorithm.
AZERO ON	no	yes	AZERO ON OK	Turns on the auto-zeroing algorithm (this algorithm must not be used on CO ₂ sensors).
CALB AAAA	no	yes	CALB AAAA OK or CALB AAAA FAULT	This command is used for gas span calibration, where AAAA is a CGM concentration value in % vol. × 100. For example, AAAA = 0198 corresponds to 1.98 % vol. See Appendix D.1 for detailed procedure description.
CALB1 XXXXX	no	yes	CALB1 XXXXX OK or CALB1 XXXXX FAULT	Writes scale coefficient for sensor calibration range of 0...5 % vol. XXXXX is the coefficient value incremented to 10000 (for example: to write the scale coefficient of 0.009 send <CALB2 00090>). This command can be used to recalibrate sensor if scale coefficient is known. The scale coefficients for different gases are individual for each sensor. To achieve cross-coefficients contact support.
CALB2 YYYYY	no	yes	CALB2 YYYYY OK or CALB2 YYYYY FAULT	Writes scale coefficient for sensor calibration range of 5...100 % vol. YYYYY is the coefficient value incremented to 10000 (for example: to store the scale coefficient of 0.01 send <CALB2 00100>). This command can be used to recalibrate sensor if scale coefficient is known. The scale coefficients for different gases are individual for each sensor. To achieve cross-coefficients contact support.
CALB3 ZZZZZ	no	yes	CALB3 ZZZZZ OK or CALB3 ZZZZZ FAULT	Writes scale coefficient for the whole sensor calibration range (0...100% vol.). ZZZZZ is the coefficient value incremented to 10000 (for example: to store the scale coefficient of 0.7 send <CALB3 07000>). This command can be used to recalibrate sensor if scale coefficient is known. The scale coefficients for different gases are individual for each sensor. To achieve cross-coefficients contact support.

Request syntax	USER mode	OEM mode	Response description	Command description
DATEZC?	yes	yes	DD.MM.YY	Returns date of the last span calibration operation.
DATEZC DD.MM.YY	no	yes	DATEZC DD.MM.YY OK or DATEZC DD.MM.YY FAULT	Writes the last date of span calibration to sensor memory (DD – 00...31; MM – 0...12; YY – 00...99).
INIT	no	yes	INIT OK or INIT FAULT	Resets sensor to the factory calibration settings. It initializes zero and scale coefficients setting them to one ("1"). After sending this command, it is recommended to check sensor readings. In case if sensor does not comply to its metrological specifications, perform span calibration (see Appendix D.1)
SETC XXXXX	yes	yes	SETC XXXXX OK or SETC XXXXX FAULT	Intended for determining the current ambient temperature in Celsius degrees (XXXXX stands for degrees; i.e. 00023 = 23 °C). Sensor writes current temperature ADC value to its memory.
UPLOAD	no	yes	U_OK	By this command, sensor is set to firmware updating mode. This mode switches off automatically upon the firmware is updated. To switch it off manually reset sensor power supply.
ZERO	no	yes	ZERO OK or ZERO FAULT	Writes current temperature ADC value and ratio S_t value to sensor controller memory by this command.
ZERO0	no	yes	ZERO0 OK or ZERO0 FAULT	Erases temperature coefficients previously defined by user.
ZERO2	no	yes	ZERO2 OK or ZERO2 FAULT	Intended for zeroing sensor. It initiates calculation and storing of the unifying zero coefficient within sensor memory. C and C_1 values are zeroed and ratio S_{tz} becomes equal 1 by this command.
INDSIG?	yes	yes	INDSIG ON or INDSIG OFF	Intended for checking the current mode displaying of sensor status with negative values in concentration field.

Request syntax	USER mode	OEM mode	Response description	Command description
INDSIG OFF	no	yes	INDSIG OFF OK	Turns off displaying of sensor status with negative values in concentration field.
INDSIG ON	no	yes	INDSIG ON OK	Turns on displaying of sensor status with negative values in concentration field (see Table 13).
USERDATA?	yes	yes	Contains 59 bytes of information and "0D" symbol.	Returns all the ten numbers contained in user section of sensor memory separated from each other with "0D" symbol.
USERDATAXX?	yes	yes	Contains 5 bytes of information and "0D" symbol	Returns a number contained in cell XX (00...09) of sensor memory user section.
USERDATAXX YYYYY	no	yes	USERDATAXX YYYYY OK	Writes a number YYYYY (00000...99999) to cell XX (00...09) of sensor memory user section.

Table 13. Negative values in concentration field while "INDSIG" mode is on

Concentration value in ASCII format	Concentration value in hex format	Description	Recommendations
-0001	8001	Sensor is warming up. After power up, measured concentration value is displayed after 40 s, but sensor metrological properties are provided only after 120 s.	Do not perform span calibration.
-0002	8002	Zero shifts to negative value.	Possibility of condensed moisture on optical elements. Dry sensor. After drying, if this status lasts longer than for 20 minutes at stable conditions, perform zeroing (see Appendix D.1 for procedure description).
-0003	8003	Dynamic temperature mode; zero shifts to negative value.	Do not perform span calibration or zeroing.

Appendix C.2.5. Commands for configuring net address

Request syntax	USER mode	OEM mode	Response description	Command description
! **	no	yes	4 bytes in ASCII format: "0D" symbol, sensor's hexadecimal net address in range 00...FF and "0D" symbol.	Returns sensor's net address
%AABB	no	yes	Three bytes in ASCII format: sensor's new hexadecimal net address and "0D" symbol.	Intended to assign a new net address AA to sensor with address BB .
NETOFF	no	yes	NETOFF OK or NETOFF FAULT	Cancels storing of sensor's net address in sensor memory. After sensor receives this command and sensor power resets, sensor's net address becomes "00".
NETON	no	yes	NETON OK or NETON FAULT	Allows assigning and storing sensor's net address by using <%AABB> command.

APPENDIX D. SENSOR CONFIGURATION

Appendix D.1. Zeroing and span calibration

Span calibration is necessary during sensor's initial installation as well as during the period of preparation for the equipment checking. It is required to perform span calibration at least once in 30 months. Manual zeroing must be performed before span calibration, after prolonged storage without power supply, after transportation as well as after dust filter is applied. It is also recommended to perform manual zeroing when status-word "31" shows up (see Appendix F, Table 17 and Table 18). For the list of CGMs necessary for span calibration, see Table 14, Table 15 and Table 16.



1. Covering sensor diffusion holes increases response time (T90).
2. Before span calibration operation, it is recommended to send command <INIT> for calibration and zeroing coefficients initialization.
3. While span calibration is being carried out, avoid:
 - excessive pressure on sensor housing,
 - > 98% humidity,
 - pressure of flowing gas less than 99 kPa and more than 103 kPa;
 - temperature changes faster than by 0.6 °C/min,
 - dust ingress (if dust filter is not used),
 - data request rate more than 1 Hz.
4. Recommended gas feeding rate when using gas adapters ESAT.200210.00:
 - 100-150 mL/min for one sensor;
 - 500-600 mL/min for 50 consecutively connected sensors.
5. For CO₂ sensors perform zeroing manually at least once in 3 months.

Zeroing and span calibration should be carried out by qualified personnel outside of an explosive area under normal conditions in the following sequence:

1. Communicate sensor via UART interface (example based on MIPEX-02/03 interface board ESAT.200200.00 is shown on Fig. 14; gas adapter ESAT.200210.00 is available as an option).
2. Auto-zeroing procedure of sensor concentration readings starts automatically during sensor self-diagnostics after power is switched on. Sensor self-diagnostics runs constantly while power is on. Use the following commands to control the algorithm: <AZERO ON>, <AZERO OFF> and <AZERO?> (this algorithm must not be used on CO₂ sensors). However, if zero shifts anyway, it is recommended to **perform zeroing manually**:
 - 2.1. within 5 minutes after power was supplied start feeding CGM #1 (high purity nitrogen) into sensor atmosphere;
 - 2.2. one minute after CGM #1 was supplied, send command <ZERO2>; thus, sensor readings on the concentration will be set to zero;
 - 2.3. stop feeding CGM #1 into sensor atmosphere;
 - 2.4. manual zeroing complete.

3. Start feeding CGM #2 into sensor atmosphere.
4. One minute after CGM #2 was supplied, send <CALB AAAA> command, where AAAA is a value of CGM concentration (e.g. value 0198 corresponds to 1.98% vol.). Thereafter scaled concentration value C_1 becomes equal to the sent value AAAA. Scale coefficient is stored in sensor microcontroller memory until the next span calibration. Before sending command <CALB AAAA>, ensure the following conditions:
 - 4.1. entered concentration value must not deviate from the current readings of more than 20 times and also must not be less than 11:

$$(C \cdot 20 > C_1 > C \cdot 0.05) \ \&\& \ C > 10$$
 - 4.2. CGM must contain more than 0.2% vol. of target gas;
 - 4.3. if these conditions are not met, sensor responds "CALB AAAA FAULT".
5. Stop feeding CGM #2 into sensor atmosphere.
6. Feed CGM #3 into sensor atmosphere and check sensor readings.
7. For methane sensors calibrated up to 100% vol. repeat the procedure steps 3, 4 and 5 with CGM #4.

If requirements to sensor readings variation are not met in accordance with Table 6, zeroing and span calibration procedure should be repeated. In case of the repeated mismatch between sensor readings and target gas concentration value in CGM #3, sensor should be sent to the manufacturer for repair or replacement.

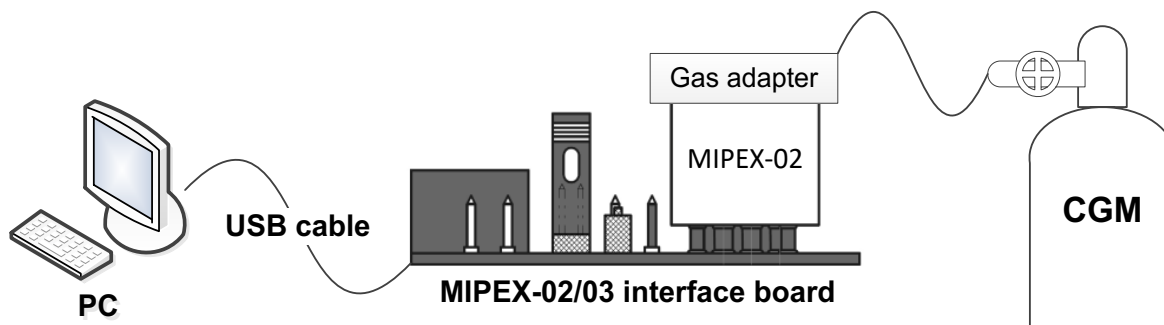


Fig. 14. Typical scheme of MIPEX-02 span calibration

Converting of % vol. to % LEL is performed according to the following equation:

$$LFSCl = \frac{100 \times C}{C(h)},$$

where:

LFSCl is component concentration, % LEL;

C is component concentration, % vol.;

C(h) is the lower explosive limit of component, % vol. (constant);

For methane C(h) = 4.4% vol.; for propane C(h) = 1.7% vol.

Table 14. CGMs used for CH₄ span calibration

CGM number according to text	Components composition	Content of methane, % vol. (% LEL)	Permissible deviation limits, % vol.	Limits of permissible error of qualification, % vol.	A number as listed in the State Register or in the Standard designation
1	N ₂	0	–	–	ISO 2435-73
2	CH ₄ , N ₂	2.2 (50)	±0.25	±0.04	ГОСТ 3883-87
3	CH ₄ , N ₂	4.15 (94)	±0.25	±0.04	ГОСТ 3883-87
4	CH ₄ , N ₂	40	±2.5	±0.4	ГОСТ 3892-87

Table 15. CGMs used for C₃H₈ span calibration

CGM number according to text	Components composition	Content of propane, % vol. (% LEL)	Permissible deviation limits, % vol.	Limits of permissible error of qualification, % vol.	A number as listed in the State Register or in the Standard designation
1	N ₂	0	–	–	ISO 2435-73
2	C ₃ H ₈ , N ₂	0.85 (50)	±0.05	±0.015	ГОСТ 5328-90
3	C ₃ H ₈ , N ₂	1.6 (94)	±0.1	±0.05	EM 06.01.648

Table 16. CGMs used for CO₂ span calibration

CGM number according to text	Components composition	Content of carbon dioxide, % vol.	Permissible deviation limits, % vol.	Limits of permissible error of qualification, % vol.	A number as listed in the State Register or in the Standard designation
1	N ₂	0	–	–	ГОСТ 9392-74
2	CO ₂ , N ₂	0.7	±0.1	±0.015	–
3	CO ₂ , N ₂	1.3	±0.1	±0.05	–
4	CO ₂ , N ₂	2.5	±0.1	±0.05	–
5	CO ₂ , N ₂	4.9	±0.1	±0.05	–

Appendix D.2. Temperature dependence of zero adjustment

It is allowed for user to adjust the temperature dependence of zero. To do this split any temperature range into equal intervals about 12.5 °C each. Each interval is used for corresponding operating temperature. Then perform the operation accordingly to an example below.

An example of procedure for temperature range of -40...+60 °C:

1. Fill sensor atmosphere with nitrogen.
2. Power on the sensor.
3. 1 minute after, send <ZERO0> command. This command erases previously defined temperature coefficients.
4. Change temperature in the range of -40...+60 °C with a pitch of 12.5 °C. For each of 9 points of temperature range, lock the temperature for at least 20 minutes.
5. When temperature is stable, for each of 9 points of temperature range send <ZERO> command, by which a current temperature ADC value and ratio S_t value (see Table 17) are written to sensor memory (see Fig. 15).

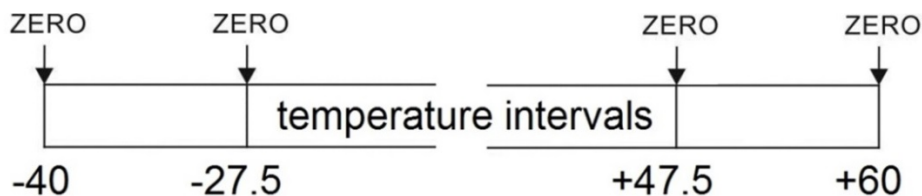


Fig. 15. Scheme of adjusting the temperature coefficients

APPENDIX E. DUST FILTER ATTACHING

To improve sensor operation reliability, dust filter should be attached to sensor surfaces. For sensor housing types “1” and “3”, only top filter (ESAT.717100.001; see Fig. 16) should be applied. For housing type “2” side filter (ESAT.717100.002; see Fig. 17) should be attached as well. Filters material is fluoroplastic membrane “Vladipor MFFC TC 6-55-221-1413-2004”. On the filter backside there is an adhesive layer “3M Double Lined Laminating Adhesive 7952” in hatched areas in Fig. 16 and Fig. 17.

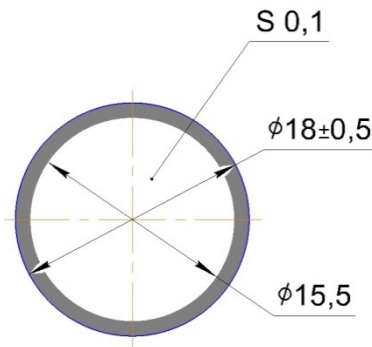


Fig. 16. Top filter dimensions

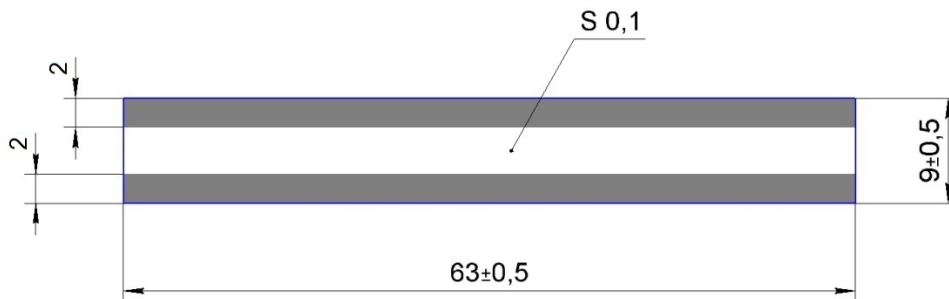


Fig. 17. Side filter dimensions

Perform the following steps to attach dust filter:



- Perform this work in a well-illuminated and well-ventilated area.
- Once a dust filter is attached to sensor surface, perform zeroing procedure (see Appendix D.1 for details).

1. Degrease surface of the upper side of sensor. For housing type “2”, perform the same operation on the side surface.
2. Extract filter from the packing and remove its substrate with tweezers.
3. Align the filter exactly to the center of the upper side of sensor with tweezers and then press on it. For housing type “2” perform the same operation on the side surface.

APPENDIX F. TROUBLESHOOTING

If there is suspicion that sensor returns wrong data and / or operates improperly, it is necessary to check its status by sending command <DATAE2> (see Appendix C.2.1). It returns concentration value and two status bytes. If any bits of status bytes are true, check their meaning in Table 12 and follow to specified recommendations. If suspicion of error or status corresponding to error persists, please contact support.

Contacting support, send log file with periodic responses to command <F>, which is intended exclusively for detailed diagnostics. It returns comprehensive information on sensor readings and its status. Sensor power consumption stated in section 6.3 is not guaranteed while using this command. Command <F> returns 72 bytes in ASCII format and "0D" symbol. Unlike <DATAE2>, it returns status word whose value corresponds to certain combination of true status byte bits (see Table 12). Detailed description of command <F> is contained in Table 17.

Sending rate of <F> command should not be more than 1 Hz.

In case if status word value is stable, log file with few (approx. 10) responses is enough. In case if status word varies eventually or periodically, log file must contain sufficient number of responses obtained before status word occurs and in time of its occurrence.

Table 17. Structure of response to <F> command

Command <F> (hex: "46 0D") response		
Byte number	Byte data	Data description
1	Hex: "0E"	Special character
2-6	T	Sensor temperature expressed in ADC counts
7	Hex: "09"	Tabulation symbol
8-12	S_t	The ratio $\frac{U_s}{U_{ref}}$ considering temperature correction
13	Hex: "09"	Tabulation symbol
14-18	U_s	Operating signal in ADC counts
19	Hex: "09"	Tabulation symbol
20-24	U_{ref}	Reference signal in ADC counts
25	Hex: "09"	Tabulation symbol
26-30	S_{tz0}	The ratio S_t considering ZERO and ZERO2 coefficients
31	Hex: "09"	Tabulation symbol
32-36	S_{tz}	The ratio S_{tz0} considering the drift compensation algorithm
37	Hex: "09"	Tabulation symbol
38-42	S_{tzkt}	The ratio S_{tz} considering the coefficient of temperature sensitivity
43	Hex: "09"	Tabulation symbol
44-48	C	Sensor readings on target gas concentration based on factory settings, % vol. × 100
49	Hex: "09"	Tabulation symbol
50-54	C_1	Scaled sensor readings on target gas concentration based on user settings, % vol. × 100
55	Hex: "09"	Tabulation symbol
56-60	Status word	Status word (see Table 18 for details)
61	Hex: "09"	Tabulation symbol
62-69	S/N	Sensor serial number
70	Hex: "09"	Tabulation symbol
71	CRC	CRC calculated using "exclusive OR" method
72	Hex: "09"	Tabulation symbol
73	Hex: "0D"	Carriage return

Table 18. Status word values description

Status word	Priority level ¹⁰	Description	Recommendations
00	12 (lowest)	Normal operating mode, temperature is static.	–
10	2	Sensor is warming up.	Do not perform span calibration.
11	3	Data request rate is more than 1 Hz.	Do not perform span calibration or zeroing. Decrease request frequency.
21	10	Dynamic temperature mode (temperature changes faster than by 0.6 °C/min).	Do not perform span calibration or zeroing.
22	9	Dynamic temperature mode (temperature changes faster than by 2 °C/min).	Do not perform span calibration or zeroing.
24	7	Dynamic temperature mode; zero shifts to negative value.	Do not perform span calibration or zeroing.
30	4	One of the signal values (U_s or U_{ref}) is lower than it is allowed	Possibility of condensed moisture on optical elements. Dry sensor. After drying, if this status lasts longer than for 20 minutes at stable conditions, replace sensor.
31	8	Zero shifts to negative value.	Possibility of condensed moisture on optical elements. Dry sensor. After drying, if this status lasts longer than for 20 minutes at stable conditions, perform zeroing (see Appendix D.1 for procedure description).
40	6	Exceeding temperature limits.	Check the ambient temperature.
50	11	An abrupt signal change (due to feeding a gas mixture to sensor atmosphere) or increased noise on sensor optical elements.	Do not perform span calibration or zeroing. If this status lasts longer than for 20 minutes at stable conditions, replace sensor.
51	5	Complex status. Technological failure.	Contact support for details
90	1 (highest)	Firmware failure (flash memory issues).	Contact support for details
1XX	–	Sensor operates in low power consumption mode.	–

NOTE: If any status word value except “00” and “21” appears, metrological properties of sensor are not provided.

¹⁰ Sensor condition is characterized by set of status word parameters. <F> command returns only one status word value in accordance with priority. To view all parameter values use command <DATAE2>.